

11-1-2019

Electrospray Photochemical Oxidation of Proteins

Remilekun O. Lawal
Louisiana State University

Fabrizio Donnarumma
Louisiana State University

Kermit K. Murray
Louisiana State University

Follow this and additional works at: https://digitalcommons.lsu.edu/chemistry_pubs

Recommended Citation

Lawal, R., Donnarumma, F., & Murray, K. (2019). Electrospray Photochemical Oxidation of Proteins. *Journal of the American Society for Mass Spectrometry*, 30 (11), 2196-2199. <https://doi.org/10.1007/s13361-019-02313-4>

This Article is brought to you for free and open access by the Department of Chemistry at LSU Digital Commons. It has been accepted for inclusion in Faculty Publications by an authorized administrator of LSU Digital Commons. For more information, please contact ir@lsu.edu.



Published in final edited form as:

J Am Soc Mass Spectrom. 2019 November ; 30(11): 2196–2199. doi:10.1007/s13361-019-02313-4.

Electrospray Photochemical Oxidation of Proteins


Remilekun O. Lawal, Fabrizio Donnarumma, Kermit K. Murray*

Department of Chemistry, Louisiana State University, Baton Rouge, Louisiana. 70803, USA

Abstract

Photooxidation of peptides and proteins by pulsed ultraviolet laser irradiation of an electrospray in the ion source of a mass spectrometer was demonstrated. A 193 nm excimer laser at 1.5 mJ pulse energy was focused with a cylindrical lens at the exit of a nano electrospray capillary and ions were sampled into a quadrupole time-of-flight mass spectrometer. A solution containing a peptide or protein and hydrogen peroxide was infused into the spray at a flow rate of 1 μ L/min using a syringe pump. The laser creates OH radicals directly in the spray which modify biomolecules within the spray droplet. These results indicate that photochemical oxidation of proteins can be initiated directly within electrospray droplets and detected by mass spectrometry.

Graphical Abstract

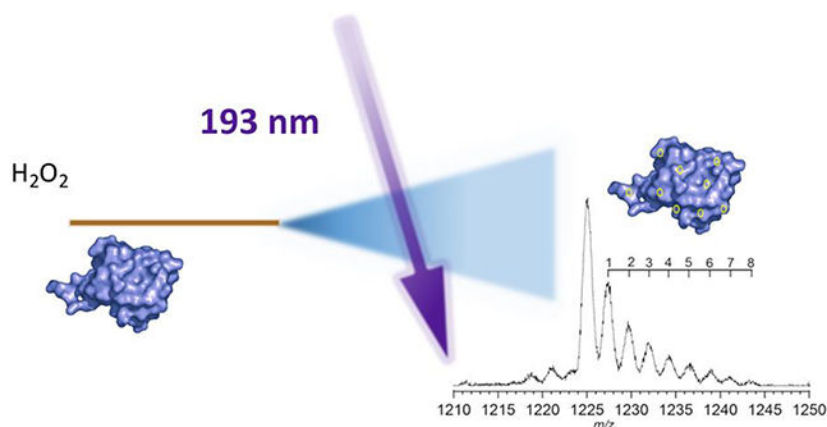

Keywords

Fast photochemical oxidation of proteins; FPOP; Electrospray; Excimer; Ultraviolet

*Corresponding Author and reprint requests: Dr. Kermit K. Murray, 331 Choppin Hall, Department of Chemistry, Louisiana State University, Louisiana, 70803, United States, Phone: +1 (225) 578-3417, Fax: +1 (225) 578 3458, kkmurray@lsu.edu.

Publisher's Disclaimer: This Author Accepted Manuscript is a PDF file of a an unedited peer-reviewed manuscript that has been accepted for publication but has not been copyedited or corrected. The official version of record that is published in the journal is kept up to date and so may therefore differ from this version.

Introduction

Electrospray droplets can be used both as a source of ions as well as for compound extraction and chemical reactions. The highly charged electrospray droplets serve as small reaction vessels that can be probed by mass spectrometry. With extractive electrospray ionization (EESI), the charged electrospray droplets merge with neutral aerosol particles containing analyte molecules that are extracted to form ions [1–5]. Reactions can be induced in electrospray droplets by exposing them to gaseous reagents. For example, hydrogen/deuterium exchange is observed in proteins within electrospray droplets when the spray is exposed to a deuterating reagent such as D₂O [6, 7] and exposure of electrospray droplets to gas phase acid or base can be used to manipulate protein charge state distribution [8, 9]. Solutions can be mixed in the electrospray cone using microfluidic channel sprayers [10] or dual channel electrospray emitters such as theta capillaries [1] or coaxial fluidic devices [11]. Reactions with lifetimes as short as 1 μs can be monitored [12] and examples include protein folding [12–14], thermal denaturation [15], and H/D exchange [1, 11, 16]. Photochemical reactions can be initiated in the electrospray using a continuous light source directed at the spray tip [17–19].

Protein footprinting is the process of chemically modifying solvent-exposed regions of proteins in their native state followed by digestion and analysis by mass spectrometry to probe the higher order structure [20]. Proteins can be oxidized in an electrospray using high voltage and an oxygen nebulizing gas [21, 22]. The resulting spray contains modified proteins that can be analyzed directly in the mass spectrometer or collected for digestion and off-line tandem mass spectrometry. Alternatively, fast photochemical oxidation of proteins (FPOP) for protein footprinting uses a pulsed UV laser to produce hydroxyl radicals from hydrogen peroxide [23–25]. The OH radicals rapidly oxidize the protein and subsequent digestion and mass spectrometry can reveal the portion of the molecule that was exposed in solution. With the use of radical scavengers, the lifetime of the footprinting process can be as low as microseconds which allows the probing of protein structure in the native state. Protein footprinting has been used for a number of applications including epitope mapping and the analysis of conformations for protein therapeutics [26].

In this work, we describe the photochemical oxidation of peptides and proteins directly in the electrospray ion source of a mass spectrometer using a 193 nm excimer laser. The electrospray contained peptide or protein standards and hydrogen peroxide and was irradiated with the laser to produce hydroxyl radicals in the spray droplet that subsequently oxidized the electrosprayed biomolecules. Spectra from oxidized and non-oxidized molecule were obtained from infusion of the same sample.

Experimental

A quadrupole time-of-flight mass spectrometer (QStar-XL, Applied Biosystems, Framingham, MA) equipped with a nanoelectrospray ion source and a custom spray tip was used for mass spectrum acquisition in positive ion mode. A schematic of the system is shown in Figure S1 of the supplemental information. The electrospray emitter was made from a 50 μm ID, 360 μm OD fused silica capillary (Polymicro Technologies, Phoenix, AZ,

USA) pulled manually after exposure to the flame of a butane torch to a ca. 10 μm inner diameter tip. The emitter was positioned 5 mm from the MS inlet and a potential of 4500 V was applied to achieve a stable electrospray. The analyte solution was infused through the capillary using a syringe pump (Cole-Parmer, Vernon Hills, IL, USA) at a flow rate of 1 $\mu\text{L}/\text{min}$ unless otherwise indicated. A 193 nm wavelength ArF excimer laser (ExciStar 200, Coherent, Santa Clara, CA) was directed into the electrospray and focused using a 25 mm focal length cylindrical lens to a 0.5 mm \times 8 mm line perpendicular to the spray axis. The laser pulse energy was 1.5 mJ and the resulting laser fluence was 400 J/m². For each experiment, the electrospray was irradiated with 100 laser pulses at 20 Hz, leading to a laser irradiation time of 5 seconds per event.

Bradykinin acetate salt, insulin from bovine pancreas, ubiquitin from bovine erythrocytes, horse heart cytochrome c, hydrogen peroxide, and LC-MS grade water were purchased from Sigma-Aldrich (St Louis, MO, USA). Formic acid (99.5%, LC-MS grade) was obtained from Thermo Fisher Scientific (Waltham, MA, USA) and methanol (LC-MS grade) was purchased from EMD Millipore (Burlington, MA, USA). Analytes were dissolved in water to a concentration of 1 mg/ml and insulin solutions contained 0.1% formic acid to facilitate dissolution. The samples were vortexed until complete dissolution. All samples were further diluted to the desired concentration with a solution of methanol and water (1:1) containing 0.1% formic acid. The resulting sample solution had a pH of approximately 1.4 and all experiments were conducted under denaturing conditions. To each sample, hydrogen peroxide was added to a final concentration of 20 mM immediately before mass spectrum acquisition.

Results and Discussion

Initial experiments were conducted using a 10 μM solution of bradykinin containing hydrogen peroxide that was infused at a flow rate of 1 $\mu\text{L}/\text{min}$. Mass spectra obtained with and without laser irradiation are shown in Figure 1; five individual spectra were averaged to produce the final spectrum. The mass spectrum in Figure 1a was obtained without irradiation and shows the m/z region with the peak corresponding to the doubly-protonated peptide at 530.7 m/z and its sodium and potassium adducts at 541.8 and 549.8 m/z respectively. The mass spectrum in Figure 1b was obtained with UV irradiation. The spectrum was obtained using 20 Hz repetition rate, 1.5 mJ energy and 20 shots per mass spectrum and five individual spectra were averaged to produce the final spectrum. The intensity of the signal associated with $[\text{M}+2\text{H}]^{2+}$ in Figure 1b is 20% lower compared to Figure 1a. Signals associated with the addition of between 1 and 6 oxygen were detected in Figure 1b and corresponds to the oxidation of the phenylalanine and proline sites on the peptide [23, 24]. These peaks can be seen in Figure 1c which was obtained by subtracting Figure 1a from Figure 1b. The extracted ion current for the signal corresponding to the doubly protonated molecule $[\text{M}+2\text{H}]^{2+}$ and the signal corresponding to the oxidized protein $[\text{M}+\text{O}+2\text{H}]^{2+}$ in Figure 1b is shown in Figure S2. The signal from the doubly protonated molecule decreases when the laser is on accompanied with a new peak associated with the oxidized molecule which is observed until the laser is shut off and the signal returns to baseline. Additionally, the intensity of the peak associated with the addition of two oxygens is greater than that from the addition of a single oxygen atom. This may result from oxidation of the two

phenylalanines, which are easily oxidized by hydroxyl radicals [27] that are likely to be at a high concentration given the 2000 fold excess of hydrogen peroxide with respect to the analyte.

The ESI voltage of 4500 V produced a stable spray without oxidizing the peptide as shown in Figure 1a. Above 5000 V, some oxidation of bradykinin was observed without laser irradiation as shown in Figure S3. Voltage lower than 4000 V resulted in unstable electrospray. The laser was directed into the Taylor cone and did not visibly affect the spray. When the laser was directed a few millimeters downstream of the Taylor cone, oxidation of the analyte was still observed but the signal was not as intense. Mass spectra acquired by varying the laser beam position relative to the MS inlet are shown in Figure S4. Laser energies between 0.5 and 6 mJ were tested. Energies between 1.5 and 3 mJ energy produced results comparable to those in Figure 1b whereas energies above 4 mJ produced lower signal from the protonated molecule without a significant change in the peak corresponding to the oxidized molecule. Below 1.5 mJ, the intensity of the signal from the oxidized molecule was lower than in Figure 1b. Representative mass spectra of bradykinin oxidation using varying laser energies is shown in Figure S5. At higher energy, the signal intensity of peaks from multiple oxygen addition is greater, which is consistent with a greater radical concentration anticipated at higher pulse energies.

Mass spectra of the protein ubiquitin are shown in Figure 2. A 10 μM solution of the protein in water with 20 mM H_2O_2 concentration was infused at 1 $\mu\text{L}/\text{min}$. The region of $[\text{M} + 7\text{H}]^{7+}$ is shown in Figure 2a for laser off and Figure 2b was obtained with the 193 nm laser directed at the electrospray. The spectra were obtained by averaging 10 individual mass spectra. In Figure 2b, the intensity of the peak corresponding to the protonated molecule was lower by approximately 70% with the laser on and peaks corresponding to the addition of up to 8 oxygen atoms were observed. A mass spectrum of ubiquitin obtained from a solution without H_2O_2 is shown in Figure S6.

Mass spectra obtained under similar conditions for insulin and myoglobin are shown in the Supplementary Information Figure S7 and S8, respectively. The insulin mass spectra for charge state $[\text{M} + 5\text{H}]^{5+}$ are similar to Figure 2 with a 40% decrease in the signal corresponding to the protonated protein and the addition of up to 11 oxygen upon 193 nm laser irradiation. The myoglobin solutions containing peroxide resulted in oxidation of the protein even in the absence of UV irradiation. The peaks associated with the oxidized protein were absent when myoglobin was electrosprayed without hydrogen peroxide (Figure S8).

Conclusions

Pulsed-laser initiated photochemical oxidation reactions within electrospray droplets with on-line mass spectrometry was demonstrated. Photochemical oxidation of peptides and proteins within charged electrospray droplets in the presence of hydrogen peroxide was accomplished by irradiating the spray just downstream of the Taylor cone with a pulsed 193 nm UV laser. Although both protein and water molecules absorb the laser energy at this wavelength, no evidence of fragmentation was observed. When combined with native

electrospray and tandem mass spectrometry this approach has the potential to enable in-electrospray protein footprinting. Furthermore, the approach is general and has the potential for application to additional wavelengths and other photochemical or photothermal processes. Reactions within electrospray droplets can be observed at time scales down to 1 μ s [12], which suggests that photochemical reactions can potentially be observed on these time scales.

Supplementary Material

Refer to Web version on PubMed Central for supplementary material.

Acknowledgements

This work was supported by National institutes of health grant (R21 EB-023110).

References

1. Mark L, Gill M, Mahut M, Derrick P: Dual nano-electrospray for probing solution interactions and fast reactions of complex biomolecules. *European J. Mass. Spectrom* 18, 439–446 (2012).
2. Gu H, Xu N, Chen H: Direct analysis of biological samples using extractive electrospray ionization mass spectrometry (EESI-MS). *Anal. Bioanal. Chem* 403, 2145–2153 (2012). [PubMed: 22434271]
3. Berchtold C, Bosilkovska M, Daali Y, Walder B, Zenobi R: Real-time monitoring of exhaled drugs by mass spectrometry. *Mass Spectrom. Rev* 33, 394–413 (2013). [PubMed: 24272872]
4. Koyanagi GK, Blagojevic V, Bohme DK: Applications of extractive electrospray ionization (EESI) in analytical chemistry. *Int. J. Mass Spectrom* 379, 146–150 (2015).
5. Monge ME, Harris GA, Dwivedi P, Fernandez FM: Mass Spectrometry: Recent Advances in Direct Open Air Surface Sampling/Ionization. *Chem. Rev* 113, 2269–2308 (2013). [PubMed: 23301684]
6. Takáts Z, Schlosser G, Vekey K: Hydrogen/deuterium exchange of electrosprayed ions in the atmospheric interface of a commercial triple– quadrupole mass spectrometer. *Int. J. Mass Spectrom* 228, 729–741 (2003).
7. Kostyukovich Y, Kononikhin A, Popov I, Nikolaev E: Simple Atmospheric Hydrogen/Deuterium Exchange Method for Enumeration of Labile Hydrogens by Electrospray Ionization Mass Spectrometry. *Anal. Chem* 85, 5330–5334 (2013). [PubMed: 23647106]
8. Kharlamova A, Prentice BM, Huang T-Y, McLuckey SA: Electrospray Droplet Exposure to Gaseous Acids for the Manipulation of Protein Charge State Distributions. *Anal. Chem* 82, 7422–7429 (2010). [PubMed: 20712348]
9. Kharlamova A, McLuckey SA: Negative Electrospray Droplet Exposure to Gaseous Bases for the Manipulation of Protein Charge State Distributions. *Anal. Chem* 83, 431–437 (2011). [PubMed: 21141935]
10. Prudent M, Rossier JS, Lion N, Girault HH: Microfabricated Dual Sprayer for On-Line Mass Tagging of Phosphopeptides. *Anal. Chem* 80, 2531–2538 (2008). [PubMed: 18318548]
11. Sundberg BN, Lagalante AF: Coaxial Electrospray Ionization for the Study of Rapid In-source Chemistry. 1–7 (2018).
12. Mortensen DN, Williams ER: Ultrafast (1 μ s) Mixing and Fast Protein Folding in Nanodrops Monitored by Mass Spectrometry. *J. Am. Chem. Soc* 138, 3453–3460 (2016). [PubMed: 26902747]
13. Mortensen DN, Williams ER: Investigating Protein Folding and Unfolding in Electrospray Nanodrops Upon Rapid Mixing Using Theta-Glass Emitters. *Anal. Chem* 87, 1281–1287 (2014). [PubMed: 25525976]
14. Fisher CM, Kharlamova A, McLuckey SA: Affecting Protein Charge State Distributions in Nano-Electrospray Ionization via In-Spray Solution Mixing Using Theta Capillaries. *Anal. Chem* 86, 4581–4588 (2014). [PubMed: 24702054]

15. Zhao F, Matt SM, Bu J, Rehrauer OG, Ben-Amotz D, McLuckey SA: Joule Heating and Thermal Denaturation of Proteins in Nano-ESI Theta Tips. 1–10 (2017).
16. Jansson ET, Lai YH, Santiago JG, Zare RN: Rapid Hydrogen–Deuterium Exchange in Liquid Droplets. *J. Am. Chem. Soc* 139, 6851–6854 (2017). [PubMed: 28481522]
17. Arakawa R, Lu J, Yoshimura A, Nozaki K, Ohno T, Doe H, Matsuo T: Online Mass Analysis of Reaction Products by Electrospray Ionization. Photosubstitution of Ruthenium(II) Diimine Complexes. *Inorg. Chem* 34, 3874–3878 (1995).
18. Ding W, Johnson KA, Kutal C, Amster IJ: Mechanistic Studies of Photochemical Reactions with Millisecond Time Resolution by Electrospray Ionization Mass Spectrometry. *Anal. Chem* 75, 4624–4630 (2003). [PubMed: 14632073]
19. Chen S, Wan Q, Badu-Tawiah AK: Picomole-Scale Real-Time Photoreaction Screening: Discovery of the Visible-Light-Promoted Dehydrogenation of Tetrahydroquinolines under Ambient Conditions. *Angew. Chem* 128, 9491–9495 (2016).
20. Takamoto K, Chance MR: Radiolytic protein footprinting with mass spectrometry to probe the structure of macromolecular complexes. *Annu. Rev. Biophys. Biomol. Struct* 35, 251–276 (2006). [PubMed: 16689636]
21. Maleknia SD, Chance MR, Downard KM: Electrospray-assisted modification of proteins: a radical probe of protein structure. *Rapid Commun. Mass Spectrom* 13, 2352–2358 (1999). [PubMed: 10567934]
22. Maleknia SD, Downard KM: Radical approaches to probe protein structure, folding, and interactions by mass spectrometry. *Mass Spectrom. Rev* 20, 388–401 (2001). [PubMed: 11997945]
23. Zhang MM, Rempel DL, Gross ML: A Fast Photochemical Oxidation of Proteins (FPOP) platform for free-radical reactions_ the carbonate radical anion with peptides and proteins. *Free Radic. Biol. Med* 131, 126–132 (2019). [PubMed: 30502457]
24. Li KS, Shi L, Gross ML: Mass Spectrometry-Based Fast Photochemical Oxidation of Proteins (FPOP) for Higher Order Structure Characterization. *Acc. Chem. Res* 51, 736–744 (2018). [PubMed: 29450991]
25. Hambly DM, Gross ML: Laser flash photolysis of hydrogen peroxide to oxidize protein solvent-accessible residues on the microsecond timescale. *J. Am. Soc. Mass Spectrom* 16, 2057–2063 (2005). [PubMed: 16263307]
26. Li J, Chen G: The use of fast photochemical oxidation of proteins coupled with mass spectrometry in protein therapeutics discovery and development. *Drug Discov Today* 24, 829–834 (2019). [PubMed: 30583089]
27. Xu G, Chance MR: Hydroxyl Radical-Mediated Modification of Proteins as Probes for Structural Proteomics. *Chem. Rev* 107, 3514–3543 (2007). [PubMed: 17683160]

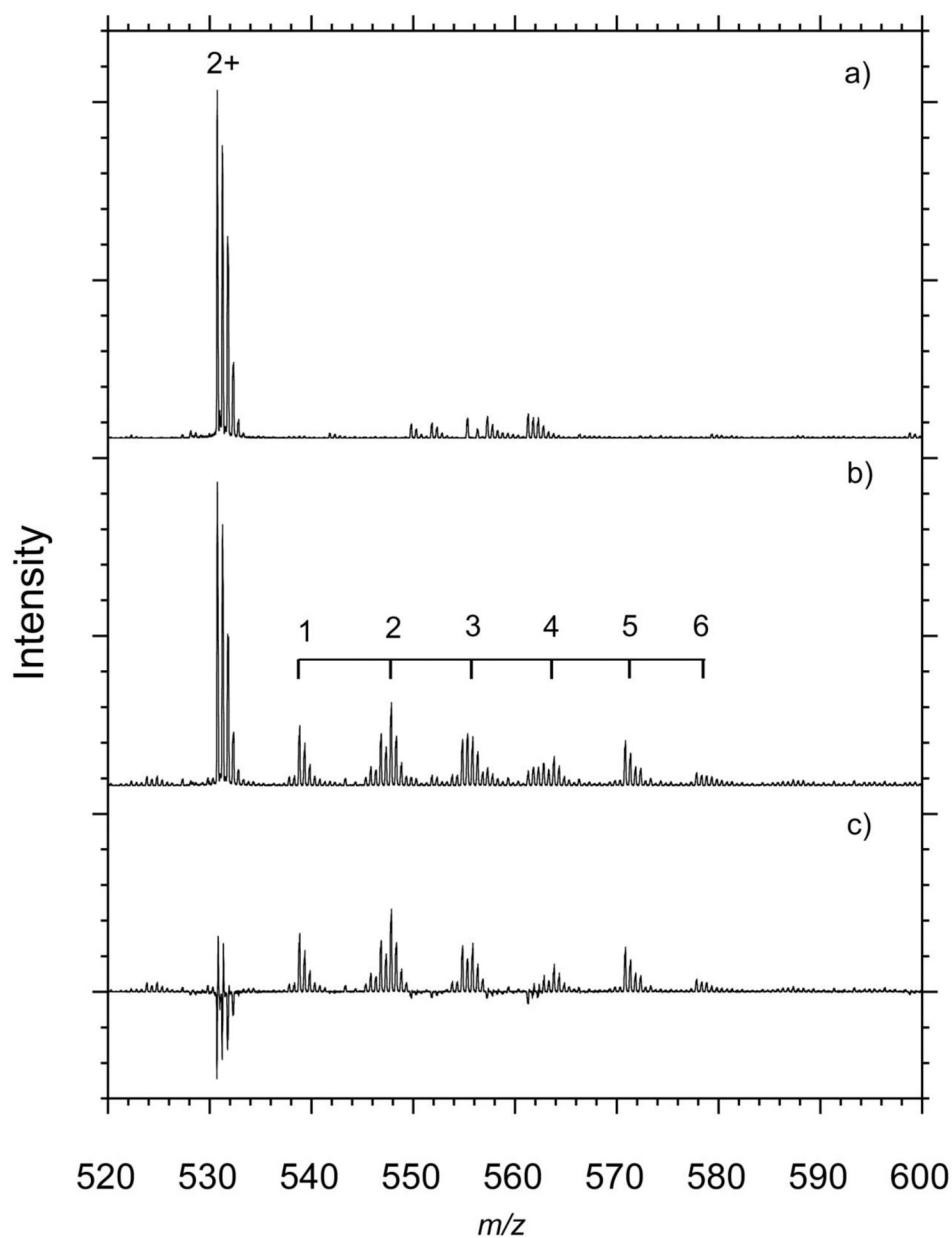


Figure 1. Representative mass spectra of +2 charge state bradykinin containing H_2O_2 acquired with a) electrospray only and b) electrospray with laser irradiation with number of oxygen addition indicated; c) laser off spectrum subtracted from laser on spectrum.

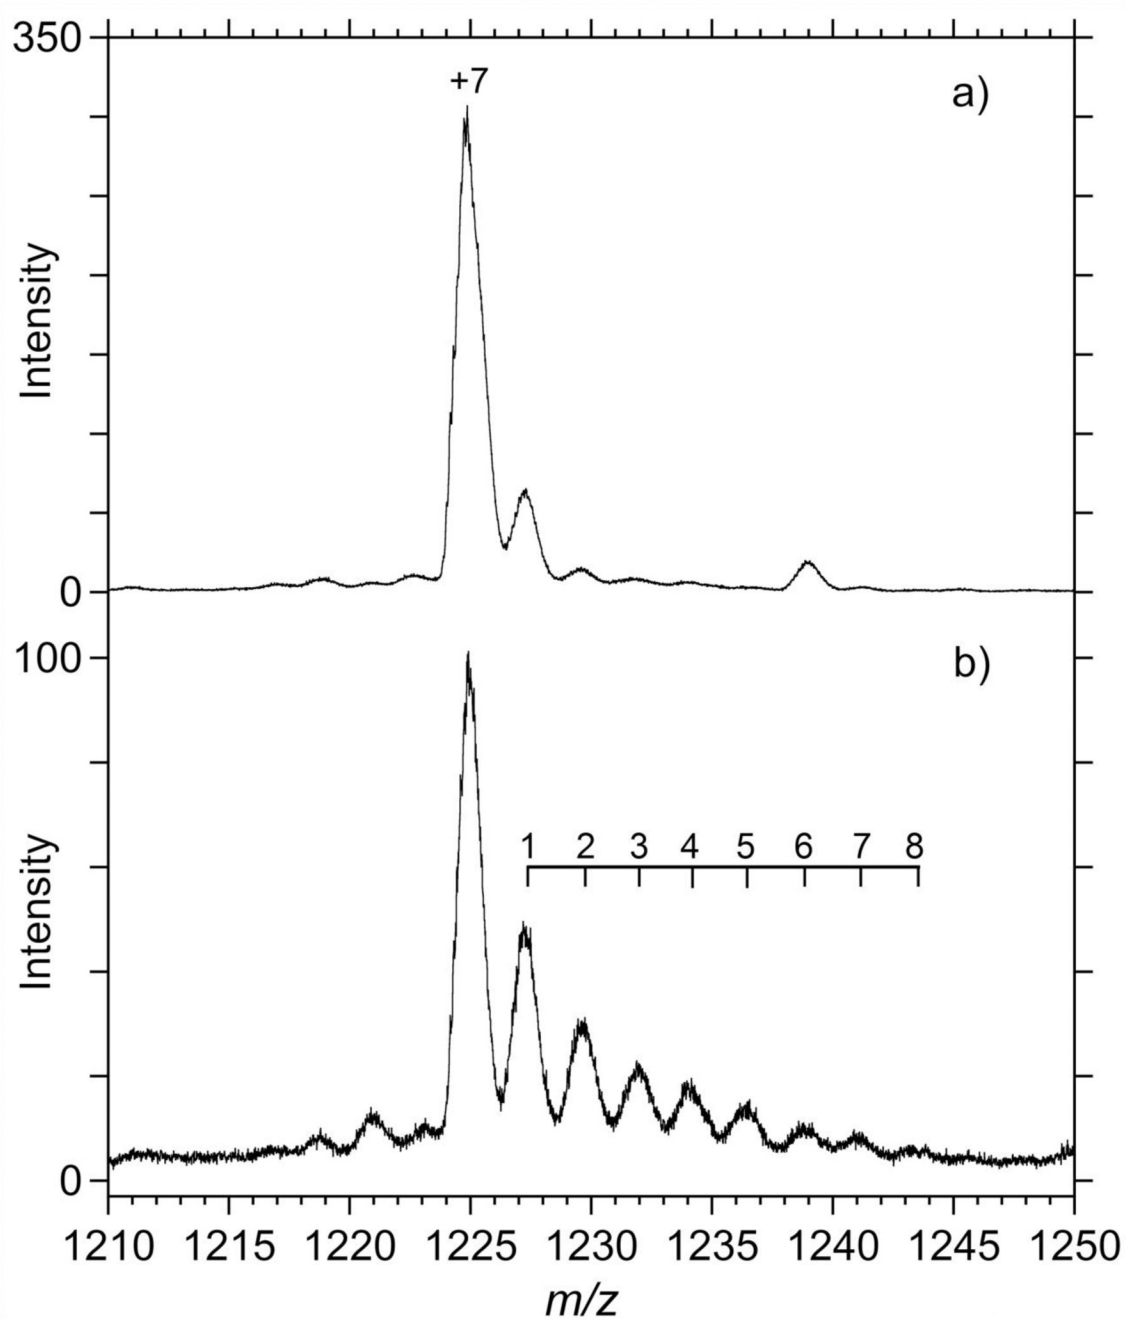


Figure 2.

Mass spectra of the +7 charge state of ubiquitin electrosprayed from an aqueous solution containing H_2O_2 acquired by a) electrospray only and b) irradiated at 193 nm.